



NATIONAL TYPE EVALUATION PROGRAM

Certificate of Conformance

for Weighing and Measuring Devices

For:

Weighing/Load Receiving Element
Load Cell, Electronic
Model: HIBS200 & HIBS300
 n_{\max} : 5000
Capacity: 5 lb e_{\min} : 0.001 lb (Model HIBS200)
Capacity: 500 lb e_{\min} : 0.1 lb (Model HIBS300)
Accuracy Class: III

***Submitted By: Contact Info. Updated November 2024**

Hardy Process Solutions
10075 Mesa Rim Road
San Diego, CA 92121
Tel: 858-255-6776
Fax: 858-675-1241
Contact: Emily Schnarr
Email: emily.schnarr@hardysolutions.com
Web site: www.hardysolutions.com

Standard Features and Options

Platform size: 8" x 8" to 30" x 30"

Construction Material Used: Stainless Steel or Carbon steel

Load Cell Used: 500 lb capacity: Teda Model 1250 (Certificate of Conformance Number 89-054A1)
5 lb capacity: Revere Transducers Model 642-A5 (Certificate of Conformance Number 93-087)

Metrologically equivalent load cells may be substituted provided no changes are made to the scale and the substitute load cells have a Certificate of Conformance.

Temperature Range: -10 °C to 40 °C (14 °F to 104 °F)

This device was evaluated under the National Type Evaluation Program and was found to comply with the applicable technical requirements of "NIST Handbook 44: Specifications, Tolerances and Other Technical Requirements for Weighing and Measuring Devices." Evaluation results and device characteristics necessary for inspection and use in commerce are on the following pages.

Ronald Hayes
Chairman, NCWM, Inc.

John Gaccione
Committee Chair, National Type Evaluation Program Committee
Issued: January 28, 2015

1135 M Street, Suite 110 / Lincoln, Nebraska 68508

The National Conference on Weights and Measures (NCWM) does not approve, recommend or endorse any proprietary product or material, either as a single item or as a class or group. Results shall not be used in advertising or sales promotion to indicate explicit or implicit endorsement of the product or material by the NCWM.

**Hardy Process Solutions**

Weighing/Load Receiving Element / HIBS200 & HIBS300

Application: The device is a single point weighing/load receiving element used in industrial and processing applications. The device can be interfaced with an NTEP certified and compatible indicating element.

Identification: The required information is on an adhesive badge attached to the scale frame.

Sealing: The weighing element has no metrological functions that require the use of a security seal. Calibration or configuration of the scale is done through the indicator.

Test Conditions: This Certificate is issued based upon the following tests and upon information submitted by the manufacturer. Two devices, 5 x 0.001 lb and a 500 x 0.01 lb, were submitted for evaluation. The emphasis of the evaluation was on the device design, operation, marking, and compliance with influence factor requirements. The scale base was interfaced with a Brechbuhler UMC 600 (CC 91-129A) indicator for the evaluation. Several increasing/decreasing load and shift tests were performed. The scale was tested over a temperature range of -10 °C to 40 °C (14 °F to 104 °F). A load of approximately one-half scale capacity was applied to the scale 100 800 times. The scale was tested periodically over this time.

Type Evaluation Criteria Used: *NIST Handbook 44 Specifications, Tolerances, and Other Technical Requirements for Weighing and Measuring Devices*, 2014 Edition. *NCWM Publication 14 Measuring Devices*, 2014 Edition.

Evaluated By: A. McCoy (OH), W. West (OH)

Conclusion: The results of the evaluation and information provided by the manufacturer indicate the device complies with applicable requirements.

Information Reviewed By: J. Truex (NCWM)




Hardy Process Solutions
Weighing/Load Receiving Element / HIBS200 & HIBS300

Examples of Device:


HIBS200



HIBS300



HIBS200 inside

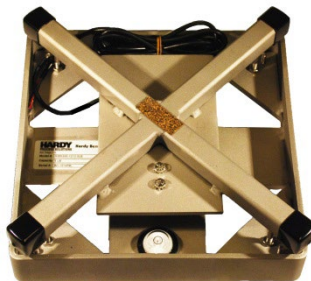

HIBS300 inside